REPUBLIKA E KOSOVËS-REPUBLIKA KOSOVA-REPUBLIC OF KOSOVA
QEVERIA E KOSOVËS-VLADA KOSOVA-GOVERNMENT OF KOSOVA
MINISTRIA E SHËNDETËSISË-MINISTARSTVO ZDRAVLJA-MINISTRY OF HEALTH
Njësia Org. Org.Jedinica Org Unit 09
Nr.Prot: Broj Prot: Prot.No: 25-8916
Nr.i faqeve Br.stranica No.pages 15
Data: Datum: Date: 15/11/2024
Prishtinë / a

Republika e Kosovës

Republika Kosova - Republic of Kosovo

Qeveria – Vlada - Government

Ministria e Shëndetësisë - Ministarstvo zdravstva - Ministry of Health

Divizioni i Prokurimit/Divizia Nabavke/Procurment Division

KONTRATË PUBLIKE

FURNIZIM

Furnizim me centrifug laboratorike për DSHB

Numri i kontratës[1]: 206-24-10999-1-3-6/C773

Numri i Prokurimit: 206-24-10999-1-3-6

GENIUS KOSOVA SH.P.K.

NUI: 811054072

[1] Ju lutemi referojuni këtij numri të kontratës në dokumentet e faturimit dhe pagesës, procedurat dhe transaksionet që lidhen me thesarin.

Numri i kontratës [2]: **206-24-10999-1-3-6/C773**

MINISTRIA E SHËNDETËSISË, (në vazhdim "Autoriteti Kontraktues"), në njërën anë; dhe

" GENIUS KOSOVA " SH.P.K., Rr.Cen Dugolli, Ferizaj, (ne vazhdim "Furnizuesi"), ne anën tjetër, janë pajtuar te lidhin një kontrate publike për furnizimet e shënuara me poshtë:

Furnizim me centrifug laboratorike per DSHB me numër identifikues: **206-24-10999-1-3-6**

Neni 1 Lënda

1.1 Lënda e kontratës do të jetë Furnizim me centrifug laboratorike për DSHB

Nr.	*Grupi*
1	**Furnizim me centrifug laboratorike per DSHB**

1.2 Kontrata hynë në fuqi me datën e nënshkrimit dhe përfundon pas 30 dite.

1.3 Afati kohor i performances nuk mund të jetë më shumë se **30** ditë nga data e marrjes së urdhëreses.

1.4 Vendi i dërgimit të furnizimeve do të jetë: **Pajisjet mjekësore do te dorëzohen neper NJSHB**

1.5 Incotermi i aplikueshëm do të jetë DDP[3] (Detyra e Dërguar e Paguar).

Neni 2 Ligji i aplikueshëm

2.1 Ligji i zbatueshëm do të jetë sipas Nenit 40 të Ligjit Nr. 04/L-042 për Prokurimin Publik të Republikës se Kosovës, i ndryshuar dhe plotësuar me ligjin Nr. 04/L-237, ligjin Nr. 05/L-068 dhe ligjin Nr. 05/L-092 Për çështjet që nuk mbulohen me dispozita të kontratës, zbatohen ligjet në fuqi në Kosovë. Juridiksioni do të jetë gjykata përkatëse në Prishtinë.

Neni 3 Çmimi

3.1 Çmimi total i kontratës do të jetë **2,700.00** Euro.

3.2 Çmimi i përmendur në Nenin 3.1 më sipër duhet të jetë e vetmja pagesë që Autoriteti Kontraktues i ka borxh Operatorit Ekonomik sipas kontratës. Ai duhet të jetë i prerë dhe të mos i nënshtrohet ndryshimeve gjatë ekzekutimit të kontratës (në përjashtim të çmimeve të atyre artikujve që i nënshtrohen ndryshimit të çmimit sipas berzës përkatëse, nëse aplikohet).

Nr. Rendor	Emertimi I Artikullit	Njësia	Sasia	ÇMIMI PËR NJËSI PA TVSH €	TVSH (%)	ÇMIMI PËR NJËSI ME TVSH €	ÇMIMI TOTAL ME TVSH €	Koha e Dërgesës max.30 ditë
1	Centrifug mjekesore per NJSHB	Copë	6	381.36	18%	450.00	2,700.00	30 Dite
						Totali (DDP):		2,700.00

Neni 4 Pagesat

4.1 Pagesa do të bëhet në Euro.

Autoriteti Kontraktues do të paguaj shumën totale te pagesës pas pranimit të tërë dërgesës

4.2 Pagesat e detyrimeve sipas një fature të lëshuar nga Operatori Ekonomik duhet të paguhet brenda jo më shumë se 30 ditësh nga data në të cilën kërkesa e pranueshme për pagesë është regjistruar nga departamenti përkatës. Data e pagesës do të jetë data në të cilën debitohet llogaria e institucionit. Kërkesa për pagesë nuk do të jetë e pranueshme nëse nuk plotësohen një ose më shumë nga kërkesat thelbësore.

---

[2] Ju lutemi referojuni këtij numri të kontratës në dokumentet e faturimit dhe pagesës, procedurat dhe transaksionet që lidhen me thesarin.

[3] DDP – Detyra e Dërguar e Paguar- Incoterms 2010 Oda Ekonomike Ndërkombëtare

Neni 5 Marrëveshjet lidhur me tatimin dhe doganën

5.1 Operatori Ekonomik është përgjegjës për të gjitha detyrimet dhe taksat në përputhje me Ligjin e Republikës së Kosovës.

5.2 Të gjitha taksat dhe detyrat e tjera doganore konsiderohen se janë të përfshira në çmimin e kontratës.

Neni 6 Kualiteti

6.1 Kualiteti i furnizimeve duhet në të gjitha aspektet të plotësoj specifikimet teknike të parashtruara në Dosjen e Tenderit.

Neni 7 Garancioni

7.1 Garancioni do të mbetet valid për 12 muaj, pas pranimit të furnizimeve.

Neni 8 Vonesat në ekzekutim

8.1 Nëse Operatori Ekonomik me përgjegjësinë e tij nuk arrin t'i dorëzojë të gjitha mallrat brenda limiteve kohore të specifikuara në kontratë, Autoriteti Kontraktues, pa njoftim zyrtar dhe pa paragjykim ndaj kompensimeve tjera të tij sipas kontratës, do të ketë të drejtë, për secilën ditë që kalon ndërmjet skadimit të periudhës së kontratës dhe datës aktuale të përfundimit, t'i marrë dëmet e likuiduara të barabarta me 0,25% në ditë të vlerës së furnizimeve të pa dorëzuara deri në një maksimum prej 10 % të vlerës totale të kontratës.

Neni 9 Inspektimi dhe testimi

9.1 Autoriteti kontraktues do të ketë të drejtë që herë pas here të inspektojë, kontrollojë, masë dhe testojë komponentët, materialet, dhe mjeshtërinë, dhe të kontrollojë përparimin e përgatitjes, fabrikimit apo prodhimit të çfarëdo artikulli që përgatitet, fabrikohet ose prodhohet për t'u dorëzuar sipas kontratës, në mënyrë që të përcaktojë nëse komponentët, materialet dhe mjeshtëria kanë cilësinë dhe sasinë e kërkuar.

Neni 10 Nën-kontraktimi

10.1 Një nënkontratë do të jetë e vlefshme vetëm nëse është një marrëveshje me shkrim me të cilin Operatori Ekonomik i beson kryerjen e një pjese të kontratës së tij një pale të tretë. Operatori Ekonomik nuk duhet të nënkontraktojë pa autorizim paraprak me shkrim nga Autoriteti Kontraktues. Autoriteti Kontraktues do të njoftojë Operatorin Ekonomik për vendimin e tij brenda 5 ditëve nga marrja e njoftimit, duke i paraqitur arsyet e veta nëse nuk lëshohet autorizimi.

Neni 11 Ndërprerja e Kontratës nga Autoriteti kontraktues

11.1 Autoriteti kontraktues mundet që, pasi t'i japë Operatorit Ekonomik shtatë ditë paralajmërim, ta ndërpresë kontratën në ndonjërin nga rastet në vijim: a) Kur operatori ekonomik nuk arrin t'i realizoj obligimet e veta sipas kontratës; b) Dështon në ekzekutimin e kontratës në afatin e caktuar; c). Refuzon urdhrat administrativ të autoritetit kontraktues; d) Ia jep dikujt kontratën apo nënkontratën pa autorizim nga autoriteti kontraktues; e). Falimenton; f). Është dënuar nga një gjykatë për një shkelje që ka të bëjë me sjellje profesionale, përmes një gjykimi që ka fuqinë e *res-judikata*; g) Operatori ekonomik i është nënshtruar një gjykimi që ka forcën e *res judicata* për mashtrim, korrupsion, përfshirje në ndonjë organizatë kriminale ose ndonjë aktivitet tjetër ilegal që i dëmton interesat e përgjithshme financiare; h) shfaqet ndonjë paaftësi tjetër ligjore që i pengon realizimit të kontratës.

Neni 12 Ndërprerja e Kontratës nga Operatori Ekonomik

12.1 Operatori Ekonomik, pasi e ka paralajmëruar Autoritetin Kontraktues 14 ditë paraprakisht, mund ta ndërpresë kontratën nëse Autoriteti kontraktues: a) Nuk arrin t'i paguajë Operatorin Ekonomik shumën që duhet të paguhet brenda periudhës së saktësuar me kontratë; b) vazhdimisht nuk arrin t'i plotësojë obligimet e veta me kontratë; c) si rezultat i forcës madhore, Operatori Ekonomik nuk është në gjendje për të kryer një pjesë materiale të kontratës për më shumë se 180 ditë, për arsye që nuk janë specifikuar në kontratë ose që nuk i atribuohen të Operatorit Ekonomik.

Neni 13 Zgjidhja e mosmarrëveshjeve me procedurë gjyqësore

13.1 Nëse nuk mund të arrihet zgjidhje brenda 30 ditësh nga fillimi i procedurës miqësore për zgjidhje të mosmarrëveshjes, secila palë mund të kërkojë ose vendim nga gjyqi, ose vendim arbitrimi.

13.2 Çdo mosmarrëveshje ndërmjet palëve të cilat mund të lindin gjatë ekzekutimit së kësaj kontrate dhe se nuk është e mundur të zgjidhet ndryshe ndërmjet palëve do të dorëzohet në gjykatën kompetente në pajtim me ligjin e Kosovës.

Neni 14 Komunikimi

14.1 Çdo komunikim me shkrim në lidhje me këtë Kontratë ndërmjet Autoritetit Kontraktues dhe Operatorit Ekonomik duhet jap Titullin e kontratës dhe numrin e i identifikimit, dhe duhet të dërgohet me postë, faks, e-mail ose me dorë.

E hartuar në gjuhen Shqipe 4 në tri origjinale, dy origjinale për Autoritetin Kontraktues dhe një origjinal për Operatorin Ekonomik.

Për Operatorin Ekonomik		**Për Autoritetin Kontraktues**	
Emri:	Besim Heziri	**Emri:**	**Berat Marmullaku**
Pozita:	MENAXHER	Pozita:	Udhëheqës Div. Prokurimit
Nënshkrimi:		Nënshkrimi:	
Data:	14.11.2024	Data:	14.11.2024
Vula:		Vula:	

[4] Gjuha do të jetë gjuha e përdorur nga tenderuesi në tenderin e tij.

Seksioni II. Formulari i PËRSHKRIMIT TË ÇMIMIT

Nr. Rendor	Emertimi I Artikullit	Njësia	Sasia	ÇMIMI PËR NJËSI PA TVSH €	TVSH (%)	ÇMIMI PËR NJËSI ME TVSH €	ÇMIMI TOTAL ME TVSH €	Koha e Dërgesës max.30 ditë
1	Centrifug mjekesore per NJSHB	Copë	6	381.36	18%	450.00	2,700.00	30 Dite
							Totali (DDP):	2,700.00

Identifikimi i Operatorit Ekonomik

Emri i Kompanise	Genius Kosova Sh.p.k.
Adresa e Plote	Rr.Bajram Kelmendi , Ferizaj
Perfaqesuar Nga:	
Emri	Valdete Neziri
Pozita	Drejtor
Nenshkrimi	
Data	29.10.2024
Vula	

Prokurimi: 206-24-10999-1-3-6

Nr i brendshëm:

Tituli: Furnizim me centrifug laboratorike per DSHB

1 Furnizim me centrifug laboratorike per DSHB

Kodi i tenderit: GK29102024

Data: 29.10.2024

Lista e dokumenteve të tenderit mbështetëse

Nr.	Dokument
1.	LICENSA.pdf
2.	qertifikata e biznesit genius kosova.pdf
3.	Autorizimi.pdf
4.	Brochura.pdf
5.	Ce.pdf
6.	Deklarata e specifikimeve.pdf
7.	Deklarata nen betim.pdf

Përshkrimi i çmimeve

Nr	Emërtimi i grupit	Dokumenti
1.	Furnizim me centrifug laboratorike per DSHB	Cmimet.pdf

Pjesët e tenderit që do të dorëzohen ndaras:

AUTORITETI KONTRAKTUES

MINISTRIA E SHËNDETËSISË, ZAGREBIT , P.N., -, PRISHTINË,

Zyrtari përgjegjes i prokurimit:

Nr i Prokurimit: 206-24-10999-1-3-6

OPERATOR EKONOMIK:

Emri i kompanisë dhe adresa e plote: **" GENIUS KOSOVA " SH.P.K., Rr.Cen Dugolli, 70000, Ferizaj, Kosovë**

E-mail: **genius.ks@outlook.com**

Personi kontaktues: **Adhurim Zejnullahu**

Telefoni: **049530030**

Faxi:

Numri fiskal: **601684302**

Grup i operatorëve ekonomik (nëse aplikohet):

FORMULAR PËR DORËZIMIN E TENDERIT

Pjesa I. Formulari i Tenderit

Numër të Prokurimit: 206-24-10999-1-3-6

Titulli i kontratës: Furnizim me centrifug laboratorike per DSHB

Si përgjigje ndaj letrës suaj të ftesës për të tenderuar për kontratën e mësipërme, ne, të poshtë nënshkruarit, deklarojmë që:

1. i kemi kontrolluar dhe pranuar plotësisht përmbajtjet e dosjes së tenderit. Ne pranojmë dispozitat e saj në tërësi, pa rezervim ose kufizim.

2. Ne ofrojmë të dorëzojmë, në pajtim me kushtet e dosjes së tenderit dhe afatet kohore të paraqitura, pa rezervë apo kufizim:

1 Furnizim me centrifug laboratorike per DSHB

3. Çmimi total i tenderit është:

2,700.00 EUR

Dhe në fjalë [*shëno çmimin e tenderit në fjalë **Euro***]

4. Ky tender është valid për një periudhë prej ose muaj: ose dite: **30** nga data finale për dorëzim të tenderëve.

5. Nëse tenderi jonë pranohet, ne marrim përsipër të sigurojmë një siguri të ekzekutimit para nënshkrimit të kontratës

6. Ne e bëjmë këtë kërkesë, për këtë tender [*shëno numrin e Pjesës, nëse aplikohet*] si partner në konsorcium të udhëhequr nga [*shëno emrin e udhëheqësit*]. Ne konfirmojmë që nuk jemi duke tenderuar për të njëjtën kontratë me ndonjë formular tjetër. Konfirmojmë, si partner në konsorcium, se të gjithë partnerët, bashkërisht dhe veç e veç, janë të detyruar me ligj për realizim të kontratës; se partneri kryesor është i autorizuar të obligojë dhe të marrë udhëzime për secilin anëtar dhe në emër të secilit anëtar që realizimi i kontratës, duke përfshirë edhe pagesat, është përgjegjësia e partnerit kryesor, dhe se të gjithë partnerët në ndërmarrjen e përbashkët/konsorcium janë të obliguar të mbeten në ndërmarrjen e përbashkët/konsorcium gjatë tërë periudhës së realizimit të kontratës.

7. Ne do ta informojmë Autoritetin kontraktues menjëherë nëse ka ndonjë ndryshim në rrethanat e mësipërme në cilëndo fazë gjatë implementimit të kontratës. Gjithashtu ne e dimë dhe pranojmë që të gjitha informatat e pasakta ose jo të plota të cilat jepen me qëllim në këtë konkurrim, mund të kenë si rezultat përjashtimin tonë nga kjo dhe nga kontratat tjera të financuara nga BKK

8. Theksojmë që Autoriteti kontraktues nuk është i obliguar të vazhdojë me këtë ftesë dhe që e rezervon të drejtën për të dhënë vetëm një pjesë të kontratës. Ai nuk do të shkaktojë detyrime ndaj

nesh nëse e bën këtë.

Informacion në lidhje me nënkontraktorët

Emri dhe adresa e nënkontraktorit	Numri fiskal - nënkontraktorë	Përshkrimi i pjesës së kontratës që do të nënkontraktohet	Pjesa vlera të nënkontraktohet	Përqindja e kontratës që do të nënkontraktohet (%)

TOPSCIEN

TOPSCIEN INSTRUMENT (NINGBO CHINA) CO.,LTD
Add:No.8 Donggong One Road, Dongguang Industrial park,
Jiangshan ,Ningbo,China
Tel:86-574-88455466 Fax:86-574-88459578
E-mail: wilsonw@topscien.com tbl@topscien.com
Http://www.topscien.com

TOPSCIEN®
www.topscien.com



laboratory Solution Supplier

INSTRUMENT

STRIVING TO BE THE LEADER IN LIQUID HANDLING INDUSTRY

Complete Product line
Laboratory Equipment And Consumables



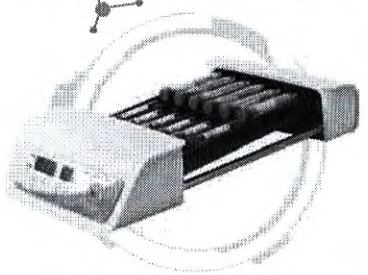

TOPSCIEN INSTRUMENT(NINGBO CHINA)CO.,LTD

STRIVING TO BE THE LEADER IN LIQUID HANDLING INDUSTRY

'High quality and reliable products, advanced service concept' is entrepreneurial business philosophy of TOPSCIEN for many years. Technology is always core competence for TOPSCIEN. There are currently more than 100 technician engaged in R&D programs. Besides, its production plants totally have approximately 1,200 technicians. The R&D headquarter in Canada includes three research institutes. Meanwhile, TOPSCIEN also establishes overseas research institutions in the United States, China and Singapore. These research institutions will further strengthen the cooperation and be dedicated to technological innovation and development of new products. They strive to make research and development to be the 'accelerator of reformation' and 'source of creation in growing' for TOPSCIEN. They also actively promote cooperation in basic and applied research with internationally renowned universities and research institutes, as well as actively promoting the development of globalization.

Its research areas are related to information communication technology, laboratory equipment, the design and development of hospital equipment, etc. Around the field of the core technology of TOPSCIEN, the member company was founded in the city of Ningbo in 2010, which sales laboratory liquid handling product, that is, Topscien Instrument (Ningbo) Co., Ltd.

ISO13485:2003 CE REACH RoHS Compliance

Micro high speed centrifuge

Feature

Extremely compact with exceptionally small footprint
12x1.5/2.0ml capacity rotor
Spin up to 14,500rpm,14,100xg
Deceleration and acceleration of< 13s
Clear, easy-to-use digital display of time and speed
Remarkably quiet operation
Metal rotor
Conform to IEC 1010-2-020 safety regulations
Separate Short Spin button for fast, convenient quick spins
Excellent air-flow minimizes heating-protects temperature-sensitive samples
Lid automatically opens at the end of the run to reduce handling time
Maintenance-free drive
Rotor is autoclavable at 121°C,20 min
Chemical resistant inner centrifuge lid

Specification

Modle	TC-MicroSpin	TC-MicroPlus
Power supply	110V-60Hz or 230V-50/60Hz	110V-60Hz or 230V-50/60Hz
Power requirement	100W	105W
Max.rotational speed (rpm)	800-13,400 rpm(in 100 rpm increments)	800-14,500 rpm(in 100 rpm increments)
Relative centrifugal force (rcf)	12,100xg	14,100xg
Timer	15 sec--99min	15 sec--99min
Acceleration time to max.speed	13s	13s
Braking time from max.speed	12s	12s
Dimensions in cm (WxDxH)	26x26x15	26x26x15
Weight (including roto)	4.3kg	4.3kg

Rotor and accessories

Transparent high strength plastiv cover

Roto high temperature and high pressure sterilization (121°C, 20min)

Optional adapter parts

----0.2ml PCR tube adapter

----0.5ml PCR tube adapter



rpm/rcf
设定相互转换

1. LCD display back lighting
2. RMP/RCF setting interconversion
3. Use the ▼▲ button setting the time and speed quickly

Order information

Cat.No.	Code No.	Specification
8011151	TC-MicroSpin	13,400 rpm/min
8011152	TC-MicroPlus	14,500 rpm/min
8011151B	TC-MicroSpin	13,400 rpm/min
8011152B	TC-MicroPlus	14,500 rpm/min

Specialise in researching and developing medical centrifuge, laboratory centrifuge, Micro centrifuge, It can meet kinds of requirement.

Nextspin Centrifuge

Nextspin SERIES centrifuge have powerful functionality, high versatility, simple operation etc features. The centrifuge suitable for extraction of medical products, blood bank, clinical trial and of blood serum, plasma, body fluids and biological specimen in biology laboratory, It is more significantly in the genetic, Protein &Nucleic Acid , PCR products field for experimental research.



Feature

Safety lid-lock, prevents opening lid until rotor stops.

DC motor free of maintenance.

Short spin and timing set spin patterns, make it more efficient.

LCD screen displays time and speed, convenient to set and read.

Use the advance and reliable CPU control system, can be control the RPM, RCF and time accurately.

Ventilation cooling system and excellent air heat exchange technology which will be reduced the rotor temperature, ensure the sample undamaged, Sound alert and automatic open the lid after the rotor stops .

Adjustable speed:100 - 5000 rpm, Max relative centrifugal force 2850xg. High accuracy of speed and time, excellent performance. More samples is dealt at one time with high efficiency.

According different kinds requirement with multiple options for selecting different kinds of centrifuge .

It include the spacer layer outside chamber for absorbing the noise, reducing the vibration; overspeed, over-current , over-voltage protection and imbalance system ensure the machine operating safety, sound alert after operating or error , the LED display show the corresponding error code .



Operation interface succinctly and clearly

Technical data

Speed Range	100~5000rpm increment: 100rpm~5000rpm
Max. RCF	2850xg
Max. Sample Capacity	8ml/5ml/3mlx24, 50mlx6
Time Range	0 ~99m,59s
Safety	Safety lid-lock, Imbalance system
Working Noise	≤ 56dB
Acceleration / Deceleration	20s↑20s↓
Power	200W

ISO13485:2003 CE REACH RoHS Compliant

NextSpin-S06

NextSpin-106

NextSpin-112

NextSpin-118

NextSpin-218

NextSpin-224

NextSpin-1524

NextSpin-S06

Order information

Cat.No.	Code No.	Specification
8011580	TC-NextSpin-218	220V 50Hz with 3ml(5ml)(8ml)vacuum tubeX18 double row angle rotor Max RCF2545xg
8011581	TC-NextSpin-218	110V 60Hz with 3ml(5ml)(8ml)vacuum tubeX18 double row angle rotor Max RCF2545xg
8011582	TC-NextSpin-118	220V 50Hz with 3ml(5ml)(8ml)vacuum tubeX18 single row rotor MaxR CF2850xg
8011583	TC-NextSpin-118	110V 60Hz with 3ml(5ml)(8ml)vacuum tubeX18 single row rotor MaxR CF2850xg
8011584	TC-NextSpin-224	220V 50Hz with 3ml(5ml)(8ml)vacuum tubeX24 double row angle rotor MaxRCF2850xg
8011585	TC-NextSpin-224	110V 60Hz with 3ml(5ml)(8ml)vacuum tubeX24 double row angle rotor MaxRCF2850xg
8011586	TC-NextSpin-112	220V 50Hz with 3ml(5ml)(8ml)vacuum tube or 15ml conical tube X12 rotor Max RCF2740xg
8011587	TC-NextSpin-112	110V 60Hz with 3ml(5ml)(8ml)vacuum tube or 15ml conical tube X12 rotor Max RCF2740xg
8011588	TC-NextSpin-106	220V 50Hz 50mlconical tube X6 angle rotor MaxRCF2740xg
8011589	TC-NextSpin-106	110V 60Hz 50ml conical tube X6 angle rotor MaxRCF2740xg
8011590	TC-NextSpin-S06	220V 50Hz 3ml(5ml)(8ml)vacuum tube or 15ml conical tube X6 swing rotor MaxRCF2510xg
8011591	TC-NextSpin-S06	110V 60Hz 3ml(5ml)(8ml)vacuum tube or 15ml conical tube X6 swing rotor MaxRCF2510xg
8011592	TC-NextSpin-1524	220V 50Hz with 15ml conical tube X24 double row angle rotor MaxRCF2850xg
8011593	TC-NextSpin-1524	110V 60Hz with with 15ml conical tube X24 double row angle rotor MaxRCF2850xg

Nextspin programmable centrifuge

Nextspin SERIES centrifuge have powerful functionality, high versatility, simple operation etc features. The centrifuge suitable for extraction of medical products, blood bank, clinical trial and of blood serum, plasma, body fluids and biological specimen in biology laboratory, it is more significantly in the genetic, Protein &Nucleic Acid , PCR products field for experimental research.



Feature

Safety lid-lock, prevents opening lid until rotor stops.

DC motor free of maintenance.

Short spin and timing set spin patterns, make it more efficient.

LCD screen displays time and speed, convenient to set and read.

Use the advance and reliable CPU control system, can be control the RPM, RCF and time accurately.

Ventilation cooling system and excellent air heat exchange technology which will be reduced the rotor temperature, ensure the sample undamaged, Sound alert and automatic open the lid after the rotor stops .

Adjustable speed:100 - 5000 rpm, Max relative centrifugal force 2850×g
High accuracy of speed and time, excellent performance
More samples is dealt at one time with high efficiency

According different kinds requirement with multiple options for selecting different kinds of centrifuge .

It include the spacer layer outside chamber for absorbing the noise, reducing the vibration, overspeed, over-current , over-voltage protection and imbalance system ensure the machine operating safety, sound alert after operating or error , the LED display show the corresponding error code .

6 sections programmable and storable
A shortcuts button for storing

技术参数/Technical data

最高转速/Speed Range	100~5000rpm 步进/increment: 100rpm~5000rpm
最大相对离心力/Max. RCF	2850xg
最大容量/Max. Sample Capacity	8ml/5ml/3mlx24, 50mlx6
定时范围/Time Range	0 ~99m,59s
安全性能 /Safety	安全门和不平衡系统/Safety lid-lock, Imbalance system
噪音 /Working Noise	≤ 56dB
加减速度/Acceleration / Deceleration	20s120s
功率/Power	200W

NextSpin-S06

NextSpin-106

NextSpin-112

NextSpin-118

NextSpin-218

NextSpin-224

NextSpin-1524

NextSpin-S06

Order information

Cat.No.	Code No.	Specification
8011650	TC-NextSpin-218	220V 50Hz with 3ml(5ml)(8ml)vacuum tubeX18 double row angle rotor Max RCF2545xg
8011651	TC-NextSpin-218	110V 60Hz with 3ml(5ml)(8ml)vacuum tubeX18 double row angle rotor Max RCF2545xg
8011652	TC-NextSpin-118	220V 50Hz with 3ml(5ml)(8ml)vacuum tubeX18 single row rotor MaxR CF2850xg
8011653	TC-NextSpin-118	110V 60Hz with 3ml(5ml)(8ml)vacuum tubeX18 single row rotor MaxR CF2850xg
8011654	TC-NextSpin-224	220V 50Hz with 3ml(5ml)(8ml)vacuum tubeX24 double row angle rotor MaxRCF2850xg
8011655	TC-NextSpin-224	110V 60Hz with 3ml(5ml)(8ml)vacuum tubeX24 double row angle rotor MaxRCF2850xg
8011656	TC-NextSpin-112	220V 50Hz with 3ml(5ml)(8ml)vacuum tube or 15ml conical tube X12 rotor Max RCF2740xg
8011657	TC-NextSpin-112	110V 60Hz with 3ml(5ml)(8ml)vacuum tube or 15ml conical tube X12 rotor Max RCF2740xg
8011658	TC-NextSpin-106	220V 50Hz 50mlconical tube X6 angle rotor MaxRCF2740xg
8011659	TC-NextSpin-106	110V 60Hz 50ml conical tube X6 angle rotor MaxRCF2740xg
8011660	TC-NextSpin-S06	220V 50Hz 3ml(5ml)(8ml)vacuum tube or 15ml conical tube X6 swing rotor MaxRCF2510xg
8011661	TC-NextSpin-S06	110V 60Hz 3ml(5ml)(8ml)vacuum tube or 15ml conical tube X6 swing rotor MaxRCF2510xg
8011662	TC-NextSpin-P1524	220V 50Hz with 15ml conical tube X24 double row angle rotor MaxRCF2850xg
8011663	TC-NextSpin-P1524	110V 60Hz with with 15ml conical tube X24 double row angle rotor MaxRCF2850xg

Spinplus Centrifuge

Spinplus-6 is the most powerful and competitive centrifuge in its class. It can be placed 6 of 15ml conical tubes or glass tubes, 8 of 15ml conical tubes or glass tubes
The speed can be100- 5000RPM, the LCD display with ability to change be between RPM and RCF.
The centrifuge is ideal for the separation of serum, plasma, urea, blood samples and other routine applications in hospital and research laboratories.

Safety lid-lock
LCD display showing
Open lid automatically
The operation interface simple and easy
RPM and RCF can be switched in display showing
8 or 6 of 15ml conical tubes with screw caps can be placed

Feature

Gentle braking at low speeds with efficient separation acceleration and braking time(20-60 seconds) can be adjustable for the 0-5000rpm speed

The LCD display with ability to change between RPM and RCF

Separate short spin button for convenient and quick spins .

Automatic release the lid when operation has stopped to save processing time

Operation can be timed from 10 seconds to 09 minutes with bell signal after finish operation

Safety lid-lock prevent opening the centrifuge lid until the rotor has stopped spinning

1 year warranty



Operation interface succinctly and clearly

Specification

Model	TC-Spinplus
Power supply	110V-60Hz or 230V-50/60Hz
Power requirement	40W
Max. rotational speed(rpm)	100-5000rpm(in 1000rpm increments)
Relative centrifugal force(rvf)	3074xg
Timer	15 sec--99min
Acceleration time to max.speed	20-80 seconds available
Braking time from max.speed	20-80 seconds available



6 tubes metal rotor



8 tubes metal rotor

订货信息/Order information

Cat.No.	Code No.	Specification
8011601	TC-Spinplus-6	220V 50Hz include the 15mlx6 rotor
8011602	TC-Spinplus-6	110V 60Hz include the 15mlx6 rotor
8011603	TC-Spinplus-8	220V 50Hz include the 15mlx8 roto
8011604	TC-Spinplus-8	110V 60Hz include the 5mlx12 roto
8011605	TC-Spinplus-12	220V 50Hz include the 5mlx12 roto
8011606	TC-Spinplus-12	110V 60Hz include the 5mlx12 roto
8011600-1	Rotor(15mlx6)	For 15mlx6(D12x75 glass tube)
8011601-2	Rotor(15mlx8)	For 15ml conical tube with screw caps
8011601-3	Rotor(15mlx12)	For 5ml conical tube with screw caps

Magic centrifuge adapter

The adjustable centrifuge adapters are ideal for properly supporting both 7ml(13 x100) and 5ml (13-75mm) tubes in a centrifuge rotor.

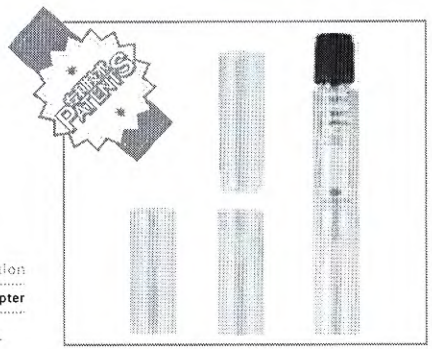

Cat.No	Code No.	Specification
8011601-8	Adapter	15ml Centrifuge adapter

Specialise in researching and developing medical centrifuge, laboratory centrifuge, mini centrifuge, it can meet kinds of requirement.

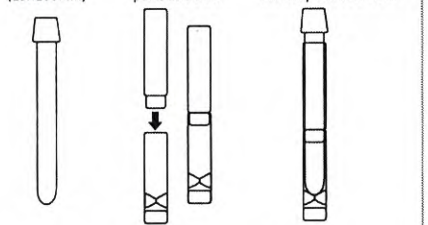

7ml Tube Configuration

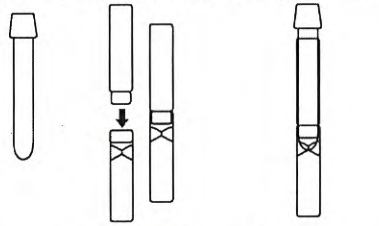

5ml Tube Configuration

Order information

Cat.No.	Part No.	Specification
8011601	TC-Spinplus-6	200V 50Hz include the 15mlX6 rotor
8011602	TC-Spinplus-6	100V 60Hz include the 15mlX6 rotor
8011603	TC-Spinplus-8	200V 50Hz include the 15mlX8 rotor
8011604	TC-Spinplus-8	100V 60Hz include the 15mlX8 rotor
8011605	TC-Spinplus-12	200V 50Hz include the 15mlX12 rotor
8011606	TC-Spinplus-12	100V 60Hz include the 15mlX12 rotor
8011601-1	Rotor(15mlX6)	For 15mlX6(D12X75 glass tube)
8011601-2	Rotor(15mlX8)	For 15ml conical tube with screw caps
8011601-3	Rotor(15mlX12)	For 5ml conical tube with screw caps

Smart Spin Microcentrifuge

SmartSpin Microcentrifuge is perfect for quick spin downs ,the Multi-Rotor can be placed 12 microtubes and /or 4 (8X0.2ml) PCR strips and the Strip –Rotor can be placed 4 (12X0.2ml) PCR strips.The Max speed can be reach 12000rpm/min.The SmartSpin Microcentrifuge is a personal centrifuge with unmatched capacity and flexibility .

Feature

Timer from 1sec-99min
Multi-Rotor for tubes and Strips
LCD display of time and speed
Double capacity of minicentrifuge
Adjustable speed from 1000rpm-12000rpm



Strips -Rotor



Multi-Rotor

Technical Data:

Capacity : 12X1.5ml / 2.0ml tubes
32X0.2ml PCR tubes
4XPCR strips (8X0.2ml)
4X PCR strips (12X0.2ml)

Speed : adjustable, 1000-12000RPM
Operating Temp : 5°C-40°C
Electrical : 100-2500V,50-60Hz 30W

Order information

Cat.No.	Part No.	Specification
8011570	SmartSpin-7	1-7Krpm/minwith mult & PCR Strips rotor
8011571	SmartSpin-12	1-12Krpm/min mult & PCR Strips rotor
8011572	SmartSpin-12	1-12Krpm/min with 5ml rotor
8011573	SmartSpin-12	1-12Krpm/min with hematocrit ,mult & PCR Strips rotor
8011570-1	Multi-Rotor	12X1.5ml/2.0 tubes &4xPCR strips (8X0.2ml) rotor
8011570-2	Strips-Rotor	4xPCR strips (12x0.2ml) rotor
8011572-1	5ML-Rotor	5ml X4 Rotor
8011573-1	HCT-Rotor	12 capillary hematocrit Rotor